



Convergence
Instruments

NSRTW_mk2

User's Manual



Oct 4 2017

Bruno Paillard

1	INTRODUCTION	3
2	APPLICATIONS	3
3	WARNINGS	4
4	GETTING STARTED	4
4.1	Software Installation	4
4.2	Hardware Installation	5
4.3	Initial Test and Configuration	5
5	INSTRUMENT FUNCTIONS AND DESCRIPTION	5
6	PRINCIPLE OF OPERATION	6
6.1	Power Consumption	6
6.2	Battery Charging	6
6.3	Modes of Operation	7
6.4	LED Indicators	7
6.4.1	Charge LED	7
6.4.2	Operation LED	8
6.5	Sound Level Calculation	8
6.6	Manual Recording	9
6.7	Automatic Recording with WiFi™ Connection	10
6.7.1	WiFi™ Connectivity	10
7	INSTRUMENT_MANAGER APPLICATION	11
7.1	Starting the Application	14
7.2	Main Functions	15
7.3	Setup Tab	15
7.3.1	Time and Date Field	15
7.3.2	Temperature Field	15
7.3.3	Instrument Info Field	15
7.3.4	Recording Field	16
7.3.5	Settings Field	17
7.3.6	Battery Field	19

7.3.7	Signals Field	19
7.4	Records Tab	20
7.4.1	Instrument Download	20
7.4.2	File Save	20
7.4.3	File Open	20
7.4.4	Exporting Data	21
7.4.5	Global Level Calculations	21
7.4.6	Graph Controls	21
7.4.7	Cursor Control	21
7.5	Spectrum Tab	22
7.5.1	Window	22
7.5.2	Weighting	22
7.5.3	Scale	23
7.5.4	Cursor, Zoom and Pan	23
7.6	WiFi Tab	23
7.6.1	Connection Status	23
7.6.2	WiFi Settings	24
7.6.3	Manual Connection	26
7.6.4	Setting Up the Server to Work in a Local or Wide Area Network.	26
7.6.5	Email Setup	26
7.6.6	WiFi™ Battery Drain	28
8	INSTRUMENT_LISTENER APPLICATION	28
8.1	File Storage	29
9	MAINTENANCE	30
9.1	Battery Care	30
9.2	Reset Procedure	30
9.3	Operation Outdoors	30
9.4	Dust	30
9.5	Cleaning	30
9.6	Software and Firmware Upgrades	30
10	TROUBLESHOOTING	31
10.1	USB Power Limitation	31
10.2	USB Driver Installation	31
10.3	Connection Problems	32

1 Introduction

NSRTW_mk2 is the second generation of Convergence Instrument's *WiFi™* enabled smart integrating sound-level meter/datalogger. It includes a type 1 digital MEMS microphone, an accurate date/time clock, a non-volatile 128 Mb recording memory and *wireless* connectivity with fast USB and *WiFi™* download.

Running on battery, it can record sound pressure levels and report them through *WiFi™* for a week. Connected to an external USB charger it can record and report for months. Its very small size allows it to be attached to or embedded within the monitored equipment.

The *NSRTW_mk2* includes the following features:

- Type I precision.
- A, C and Z weighting curves.
- *Integrating* Sound-Level Meter, records L-max, L-min and Leq levels.
- Log interval adjustable from 125 ms (8 points per second) up to hours.
- Individual Manufacturer's Certificate of Calibration from Convergence Instrument provided with every instrument purchased.
- *WiFi™* connectivity to report measured levels remotely and automatically at preset intervals.
- Open TCP/IP protocol, allows the customer to control the instrument remotely through a custom application.
- Email alarms for sound detected over specified threshold, as well as low-battery.
- Digital very sensitive MEMS microphone (30 dBA typical noise floor).
- Completely sealed weatherproof enclosure designed for outdoors applications.
- All-digital design.
- Ultra-stable sensitivity (field recalibration is easily done, but seldom required).
- Very low sensitivity variation due to temperature changes.
- Very low sensitivity to vibrations.
- Software function calculates global Leq and/or dose, according to ISO and OSHA methods.
- Adjustable response time.
- Preprogrammed recording start date/time.
- Integrated oscilloscope function that can show the acoustic signal in real time.
- Integrated spectral analyzer function that can show the spectrum (or 3rd-octave bands) in real time.
- Can be used as a high-quality USB digital microphone.
- Allows the observation of recorded levels while the recording is ongoing.
- Works standalone, or USB connected.
- Long life internal rechargeable battery that recharges from USB and most USB chargers.
- Can be field-calibrated.
- Observes and records 100% of the acoustic signal (no missed samples).
- Editable individual custom ID for easier instrument management.
- All settings are stored in non-volatile memory. So the instrument will regain full functionality and *WiFi™* connection from hard-reset or battery loss.

2 Applications

- Sound level and acoustic dose measurement and recording.
- Monitoring of safe working conditions.
- Email Alarms when the noise is too loud.
- Activity detection and logging.
- Long-term measurement and recording of acoustic levels for environmental impact studies.
- Specially designed for long-term outdoors applications.

3 Warnings



Never blow air at the microphone.



When operating in a dusty environment, take the precautions discussed in https://convergenceinstruments.com/pdf/Dust_Issues.pdf



Avoid over-discharging the battery

- Recharge the instrument immediately if the LED indicates a low-battery condition.
- Even if the instrument is idle all or most of the time, recharge it fully at least once every 6 months.
- When leaving the instrument idle for a long time, make sure the WiFi™ periodic connection is disabled.



Do not store or operate the instrument at temperatures exceeding the following limits

- -20 °C to 60 °C (-4 °F to 140 °F)



When using the instrument outdoors, make sure the USB connector is facing down. This way rain will not accumulate in the connector and microphone port.



Do not mount on a metal plate. That would drastically weaken the WiFi™ signal.

4 Getting Started

4.1 Software Installation

- On the PC that is used to setup the instrument, run *Instrument_Manager_Installer.exe*. This installs the *Instrument_Manager* application, as well as its USB driver and documentation.
- On the PC that is used as a server, to collect data over the network, run *Instrument_Listener_Installer.exe*. This installs the listener application that is used to respond to instrument's incoming connections, and create and fill the corresponding data files.

Note: The same PC can be used for both applications.

Note: Perform the software installation above BEFORE connecting the instrument to the PC for the first time.

4.2 Hardware Installation

1. Connect the instrument to an available USB port on the PC
2. Verify that the PC properly detects the instrument and loads the driver. In case of doubt see section [Troubleshooting](#).

4.3 Initial Test and Configuration

1. Upon connection to the PC, the *charge* LED should light-up yellow (charging) or green (charged). The *operating* LED should blink once per second.
2. Go into *Start\All Programs\Convergence_Instruments\Instrument_Manager* and run *Instrument_Manager.exe*. The front-panel described in [Figure 2](#) appears, and the application tries to connect to the instrument. If it fails to find the instrument it indicates *No Device Found*. If this is the case see section [Troubleshooting](#)
3. Otherwise the application switches-on the *NSRTW_mk2* and starts communicating with it.
4. If the Time and Date in the upper right corner of the application window are not properly adjusted the application asks if you want the instrument time to be synchronized to the PC time. Only say YES if the PC time is correct.
5. In addition, the application detects if the time zone of the instrument is different from the time zone of the PC. If it is, the application asks to set the instrument to the same time zone as the PC.

Note: If (in rare cases) the instrument is not intended to be used in the same time zone as that of the PC used to configure it, we suggest to temporarily change the PC's time zone to the time zone where the instrument will be recording, let the application set the instrument to the PC's time zone, and change the PC's time zone back after that initial setting. Afterwards if/whenever the application asks to change the instrument time zone back to the PC's time zone, simply choose to cancel the adjustment.

6. In the front-panel of the application you should see the acoustic signal display in real-time.

5 Instrument Functions and Description

The instrument connects to a PC on a USB port. The *Instrument_Manager* application is used to set its operating parameters and download recorded data.

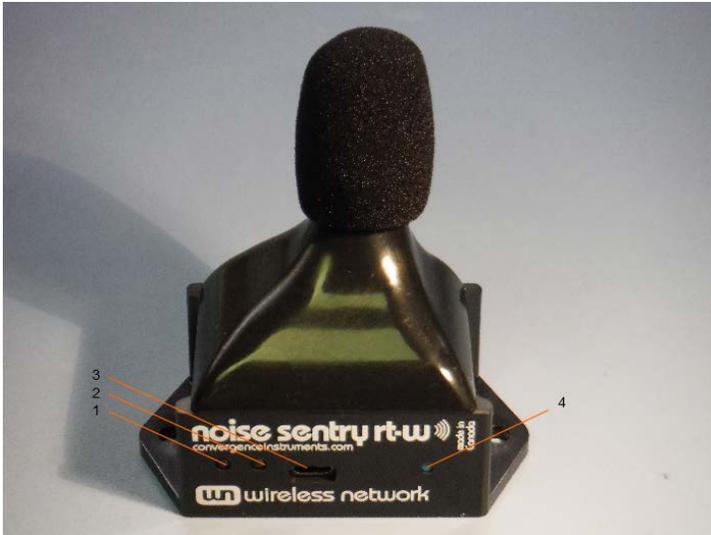


Figure 1 **Noise-Sentry-RT-W**

1. Charge LED
2. Operation LED
3. USB Connector
4. Reset Button

6 Principle of Operation

6.1 Power Consumption

The *NSRTW_mk2* is always on. However, when not in operation it only measures time, which only takes a tiny operating current. In that *Idle* state it can stay on for up to 6 months. When the *NSRTW_mk2* is actively measuring, its power consumption allows it to record for 1 week.

The *NSRTW_mk2* can be configured to connect to a server at regular intervals. When that function is enabled, the *NSRTW_mk2* will activate its *WiFi™* interface at the defined interval, and attempt to connect via *WiFi™* for up to 1 minute. During that time, the instrument's power consumption will be increased. If the connection fails the *NSRTW_mk2* will fall back to its previous state (Sleep or Recording).

Note: *WiFi™* communications consume battery, so when leaving the *NSRTW_mk2* unused for a long time, it is important to disable the *WiFi™* periodic connection feature.

In applications where the *NSRTW_mk2* must record for longer periods of time, it can be connected to a USB charger. For outdoor-use, a USB-output solar panel, such as the one found in <https://convergenceinstruments.com/product/data-logger-accessories-solar-panel/> is an ideal solution that will power the instrument indefinitely.

6.2 Battery Charging

The battery charges whenever the following conditions are met:

- The battery has not reached full charge.
- The instrument is connected to a PC's USB port and the PC is not in standby, or
- The instrument is connected to a USB charger.

While charging, the charge LED is orange. When fully charged, the LED changes to green.

The charge time from a completely discharged state varies with the amount of power the PC allows the instrument to draw. Charge time is normally around 2H30. If the PC does not allow the fast charge current, the charge time can increase up to 5 to 6 hours.

Note: When connected to a PC, battery charging stops while the PC is in standby.

Note: It is OK to leave the instrument connected to a PC or USB charger all the time. The smart charger inside the instrument will stop charging as soon as the battery reaches full-charge.

6.3 Modes of Operation

The *NSRTW_mk2* has four modes of operation:

Mode	Operation	Power Consumption
Idle	Disconnected from USB and not actively recording - Only keeps time.	Minimal: can stay on for up to 6 months.
Active	Connected to USB – Not recording – Instrument is fully on and measuring	Instrument draws power from USB to power itself, and if necessary recharge its battery. Battery is not depleted.
Recording	USB-connected or not - Fully on and recording.	If USB-connected, power comes from USB. If not, power comes from the internal battery. If not connected the instrument can record for up to 7 days.
Periodic WiFi™ Connect	From any state, including <i>Idle</i> and <i>Recording</i> , the instrument can periodically wake up its <i>WiFi™</i> interface and attempt to connect to a server. If the connection is not established after 1 minute it falls back to its original state until the next connection time.	If USB-connected, power comes from USB. If not, power comes from the battery. The <i>Periodic Connect</i> feature consumes battery. This is especially the case if the connection interval is set to be short so it occurs often.

Table 1

6.4 LED Indicators

The *NSRTW_mk2* has two LED indicators:

6.4.1 Charge LED

The charge LED is always fully on or off.

LED State	Meaning
Off	Instrument is disconnected, or is connected to a PC that is in standby.

Green	Instrument is connected to a PC or USB charger, and the battery is full.
Orange	Instrument is connected to a PC or USB charger, and the battery is charging.

Table 2

6.4.2 Operation LED

The operation LED is always blinking.

LED State	Meaning
Off	Instrument is in <i>Idle</i> mode.
1-blink/second	Instrument is in <i>Active</i> mode, but is not actively recording.
2-blinks/second	Instrument is actively recording.
1-blink/second (off-beat)	Instrument is presently communicating with a server via <i>WiFi™</i>
4-blinks/second	Battery is low. Recharge as soon as possible. If the battery level becomes critical the instrument will go to <i>Idle</i> mode (LED-off) in order to safeguard the battery against over-discharge as much as possible.

Table 3

6.5 Sound Level Calculation

After extracting the signal power, the calculated sound levels are low-pass filtered (smoothed) using an adjustable time constant. This time constant is applied to the calculation of *L-min* and *L-max*, but not *Leq*. A typical short time constant (125 ms and lower) allows the measurements to track sharp changes, while a longer time constant (1s and longer) provides more stable (cleaner) RMS values that average short transients.

The *Leq* is integrated linearly over the specified log interval, irrespective of the time constant setting.

The sound level statistics (*L-min*, *L-max* and *Leq*) are gathered for the specified *log-interval* before being written to the recording memory. The *log-interval* represents the interval at which the selected statistics are written to memory. Therefore a longer *log-interval* uses less memory, while a shorter *log-interval* provides better time resolution and allows the user to distinguish between events that occurred close together. The statistics (*L-min*, *L-max* and *Leq*) are reset at the beginning of each *log-interval*. Then the statistics are gathered sample-by-sample during the *log-interval*. At the end of each *log interval* the calculated statistics are written to memory, and the next *log-interval* is started. No portion of the signal is overlooked.

The *log interval* is set to 1 second by default. It can be set to as short as 1/8 s.

*Note: The time constant only affects the calculation of *Lmin* and *Lmax*. The *Leq* is integrated linearly over the specified log interval.*

6.6 Manual Recording

Every time a recording is started, a new record is created in memory and filled until the recording is stopped. That record is time-stamped, so the signals can be displayed with respect to absolute date/time. Records are stored sequentially in the instrument's memory. There is no limit to the number of records that the memory can contain, only a limit to the total size of the data recorded. The *Instrument_Manager* application displays the total memory recording time as a function of the various setup parameters.

After (or while) recording, the records contained in memory can be downloaded from the instrument and observed or exported. In case a recording is ongoing the last record is only displayed up to the present time.

The recording is stopped automatically when the recording memory is full. This way a new record will not overwrite an old one.

The recording memory is non-volatile, so there is no risk of losing the data that has already been recorded, even in the case of a battery failure.

Note: It is perfectly legal to find empty records in memory. That occurs typically when a recording is started and stopped quickly (for a time shorter than the log interval), before any data had time to be written to memory. In that case only the time-stamp is written to memory.

An empty record can also occur when a recording was started but no data (L_{min} , L_{max} or Leq) was selected to be recorded.

To record sound levels proceed as follows:

1. Select the statistics to be recorded (L_{min} , L_{max} and/or Leq).
2. Select the log-interval. Note that the total recording time is automatically calculated and displayed by the *Instrument_Manager* application, as a function of the log-interval and statistics selected. The log-interval is adjustable in 125 ms increments, from 125 ms up to 2H.
3. Select the time constant used to smooth the measured sound levels for L_{min} and L_{max} . Choose the Fast time constant (125 ms) to be able to detect short peaks and valleys. Choose the Long time constant (1 s) to provide cleaner more stable sound levels. Or adjust to another value, as required by the application
4. When ready to start a recording immediately, simply press the *Record* button. Press *Record* again to stop the recording.
5. Or to set a start time/date:
 - Check to make sure that the instrument time is correct. If that is not the case press the *Sync* button in order to automatically set the instrument time to the PC time.
 - Press the *Timer* button. Set a start time and date using the calendar.
 - Click OK to arm the trigger.

6.7 Automatic Recording with *WiFi*TM Connection

The *NSRTW_mk2* supports a mode of operation where it periodically connects to a server (a Windows PC running the *Instrument_Listener* application) through *WiFi*TM. This feature is designed to let the instrument record autonomously, periodically report the levels recorded since the last connection, and optionally send emails with noise-level or low-battery alerts. When set, this feature will work, even if the instrument is reset, or if it loses and regains battery power (for instance if the instrument is reconnected to a charger after the battery has been completely drained).

This PC-server being connected-to does not have to be in the vicinity of the instrument. It can be a continent apart, as long as it is reachable through the internet, and all firewalls have been set to allow the connection.

The instrument connects to a *WiFi*TM Router or *Access Point* that is in its vicinity. From there, it will find the server to connect to, either by its IP address, or by its domain name.

6.7.1 *WiFi*TM Connectivity

6.7.1.1 *WiFi*TM Reporting

*Note: When using the instrument with *WiFi*TM connectivity, do not start a recording manually, or via the timer. The instrument will be completely controlled by the server, including starting the recording, erasing memory if required, and resetting the time.*

When using the *WiFi*TM feature, the instrument will try to connect to a known server at regular intervals, or immediately in case of alarm.

Whenever it connects, the instrument will talk to a special *Instrument_Listener* application running on the server. That application will do the following:

- If the instrument was recording:
 - Upload the latest recorded data from the instrument and updates a growing file with that data (create the file if it was not already created).

- If the instrument was not recording (for instance if the recording was stopped earlier because the memory was full):
 - Upload the latest recorded data from the instrument (if any) and update the recording file.
 - Adjust the instrument time (does not adjust the time zone of the instrument, just precisely readjust the Universal-Time-Code running in the instrument).
 - Delete all data in the instrument's memory (all that data has already been safely stored in the recording file on the server).
 - Start a new recording.

6.7.1.2 Email Alarms

In addition to trying to connect to the server at regular intervals, the instrument will try to connect immediately to the email server in case of alarm. The alarm function does not require the use of a server or *Listener* application. The instrument will typically connect to an email server, such as a *gmail* account.

In order to be able to send an alarm email, the instrument must have the following setup:

- A *WiFi™* Router or *Access Point* must be in the instrument's vicinity, and the instrument must have been configured with that router's connection parameters. That is part of the *WiFi Setup* of the instrument.
- The instrument must have been configured with an outgoing email account and connection parameters. That is part of the *Email Setup* of the instrument.

Two alarms can be enabled:

- A noise level over a preset threshold.
- The battery is close to being depleted.

7 Instrument_Manager Application

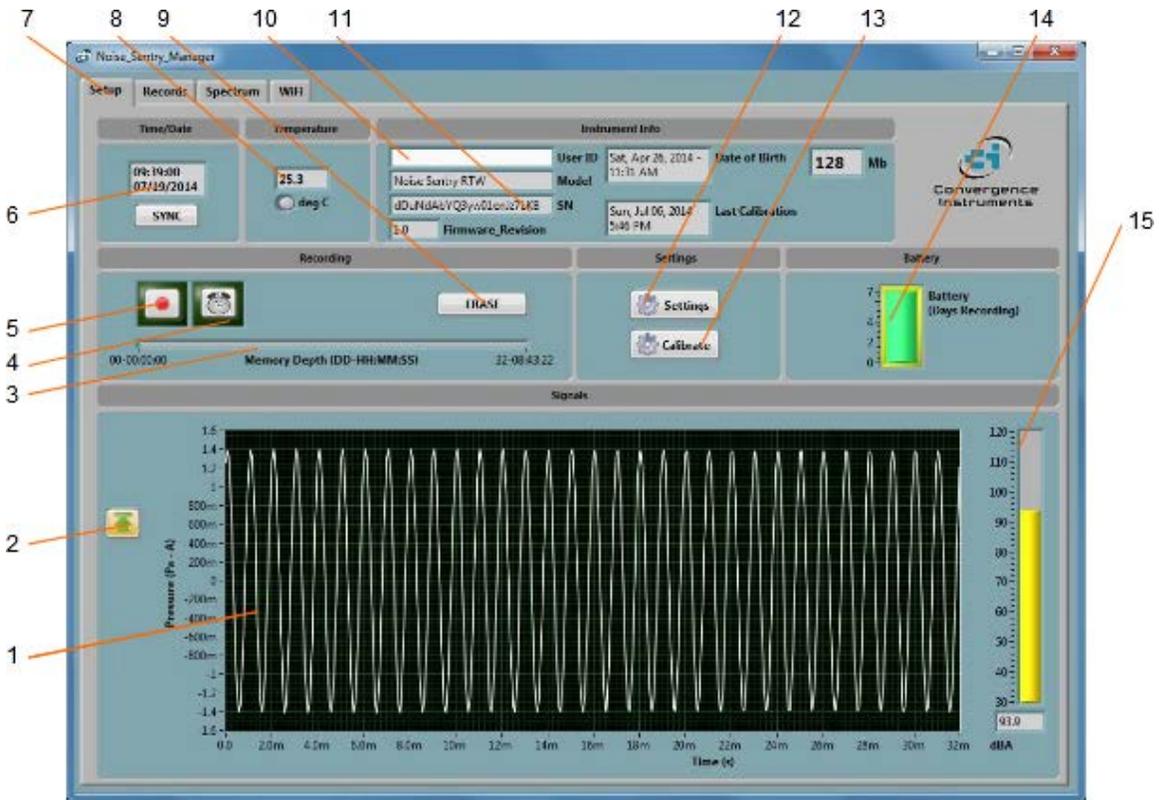


Figure 2 Setup Tab

1. Real-Time Acoustic signal
2. Auto-Range button
3. Memory fill indicator
4. Timer button
5. Record button
6. Instrument Time indicator
7. Tab selector

8. Instrument Temperature indicator
9. Erase button
10. Instrument User ID
11. Instrument Information
12. Settings button
13. Field calibration button
14. Battery Condition, Charge and Recording Time Field
15. Sound Level indicator

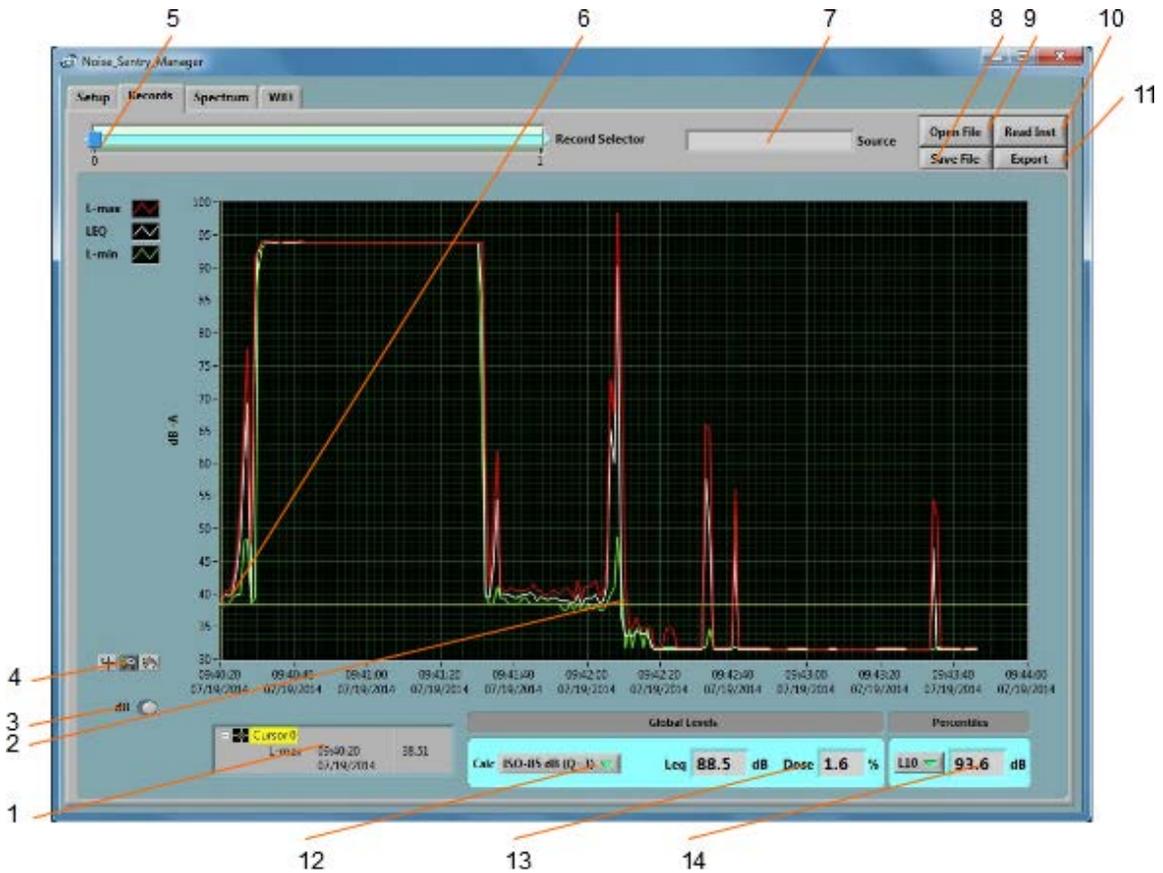


Figure 3 Record Tab

1. Cursor field
2. Recorded levels
3. dB/Lin button
4. Pan and zoom buttons
5. Record number selector
6. Cursor
7. Data source
8. File Save button
9. File Open button
10. Instrument Download button
11. Export button
12. Global level/dose calculation method
13. Global Level/Time-Weighted-Average value
14. Percentiles

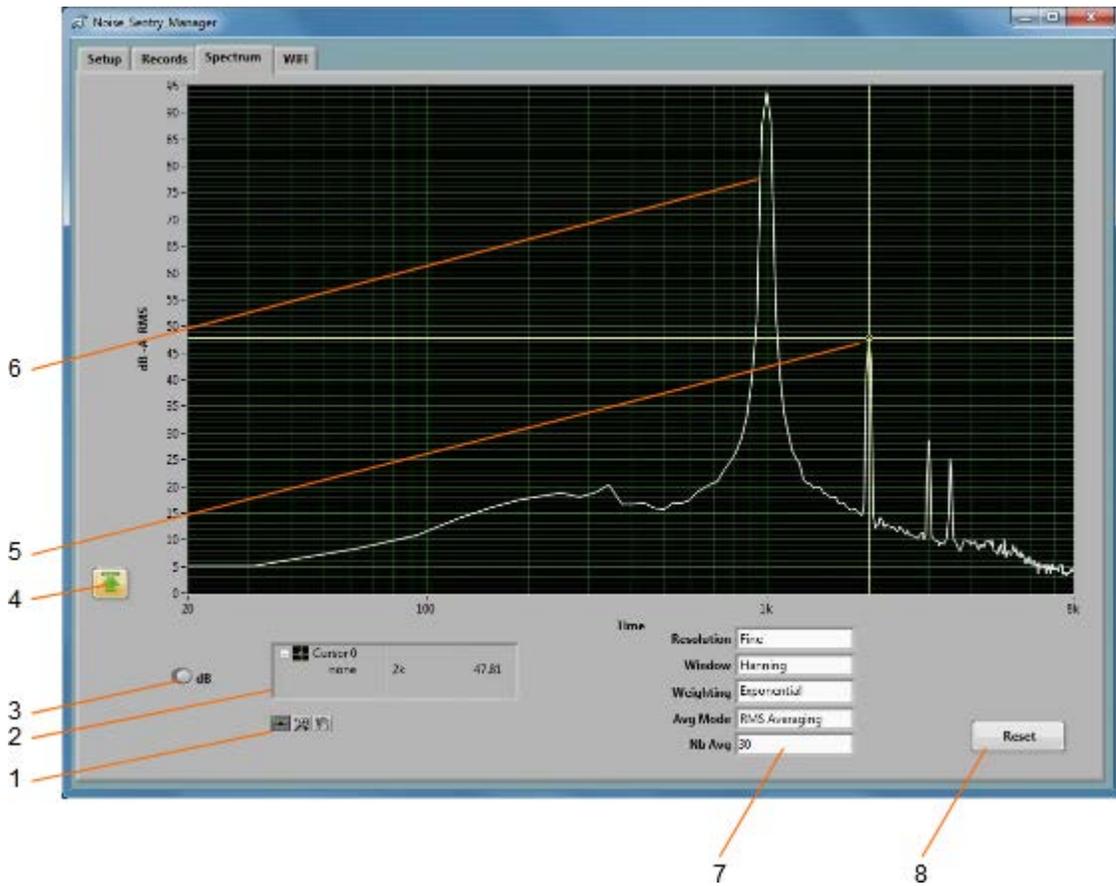


Figure 4 **Spectrum Tab**

1. Cursor, Zoom and Pan controls
2. Cursor values display
3. dB/Lin button
4. Auto-scale button
5. Cursor
6. Spectrum
7. Spectral controls
8. Spectrum reset button

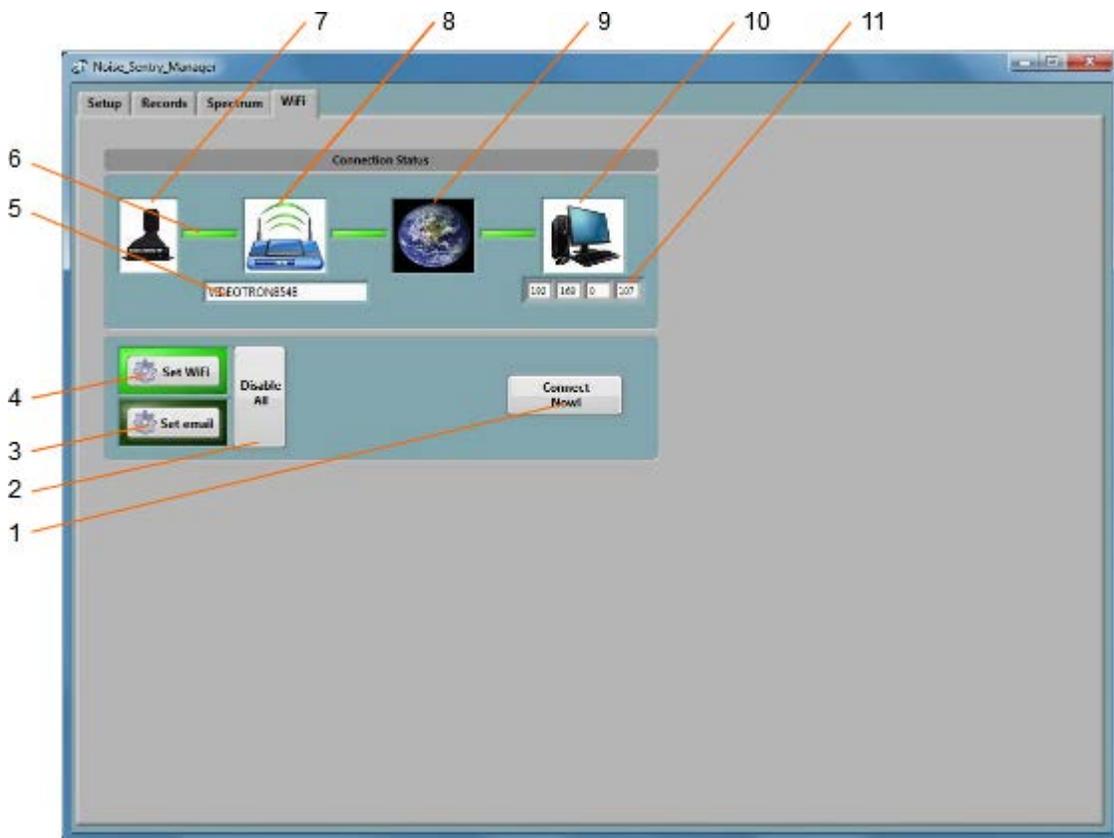


Figure 5 WiFi Tab

1. Connection Test Button
2. Disable All WiFi Button
3. Email Setup Button
4. WiFi Setup Button
5. Name (SSID) of WiFi Access Point or Router
6. Link Indicator
7. WiFi Active Indicator
8. Router or Access Point Connected Indicator
9. Network Connected Indicator
10. Server Connection Indicator
11. Server IP Address

7.1 Starting the Application

Note: The application can be run with or without an *NSRTW_mk2* connected. When an *NSRTW_mk2* is not connected the application can only be used to display and analyze a previously saved log file. All the controls and indicators related to the instrument are grayed out.

To control an *NSRTW_mk2* using the *Instrument_Manager*, proceed as follows:

1. Connect the instrument to an available USB connector on the PC.
2. Make sure that the charge LED lights-up yellow or green, and that the operation LED starts blinking. If not, review the installation procedure, or see section [Troubleshooting](#).

3. Go to `Start\All-Programs\Convergence_Instruments\Instrument_Manager`, and run `Instrument_Manager.exe`.
4. The front-panel described in [Figure 2](#) appears, and the application tries to connect to the instrument. If it fails to find the instrument it indicates *No Device Found*. If this is the case see section [Troubleshooting](#).
5. Otherwise the application immediately starts communicating with the `NSRTW_mk2`.

7.2 Main Functions

The application has four main tabs:

- **The Setup Tab:** Is used to setup the instrument and monitor real-time signal (see [Figure 2](#)).
- **The Records Tab:** Is used to download, display and export the data from the `NSRTW_mk2` (see [Figure 3](#)).
- **The Spectrum Tab:** Is used to display a real-time power spectrum from the `NSRTW_mk2` (see [Figure 4](#)).
- **The WiFi Tab:** Is used to display the present connection state of the `NSRTW_mk2`, and to setup its connection parameters (SSID, Security, Password...etc.) (see [Figure 5](#)).

7.3 Setup Tab

The setup tab is seen in [Figure 2](#). It is divided into seven fields.

7.3.1 Time and Date Field

This field displays the internal time of the instrument. If the instrument time is not properly adjusted, press *Synchronize*. This synchronizes precisely the instrument time to the PC time. Make sure the PC time is accurate before synchronizing the instrument.

Note: *Time synchronization is not allowed while the instrument is recording.*

7.3.2 Temperature Field

This field is used to display the instrument's internal temperature in °C or °F. It is normal for the internal temperature to rise slightly while the instrument is charging.

7.3.3 Instrument Info Field

The instrument info field provides instrument information, such as instrument model, serial number and firmware revision. In addition the *User-ID* field may be used to assign a custom identifier to the instrument.

To set, modify or delete the *User-ID*, simply place the cursor in the *User-ID* box and write a new identifier or clear the text. The new identifier is written to the instrument's memory as soon as *return* or *enter* is pressed, or if the mouse is left-clicked outside of the box.

The *User-ID* is written to non-volatile memory, so it is retained even in the event of a reset or battery failure.

7.3.4 Recording Field

Note: When using the instrument with WiFi™ connectivity, do not use any of the controls in the Recording field. The instrument will be completely controlled by the server, including starting the recording, erasing memory if required, and resetting the time.

The recording field has three buttons:

- **Record** The *Record* button is used to immediately create a new record and start recording. The new record is placed in memory immediately after the last one. The recording stops when the memory is full, or when the *Record* button is pressed again. The recording parameters, such as number and types of values recorded...etc. must be adjusted prior to starting the recording.
- **Timer** The *Timer* button is used to set a time and date to start the recording automatically. This is only allowed when a recording is not already in progress. To set the timer, press the *Timer* button. Then set the recording date and time, and press the *OK* button to arm the timer.
- **Erase** The *Erase* button erases unconditionally all the data that has been recorded in the instrument, making room for new records.

The *Memory Depth* bar provides two indications:

- The percentage of memory already used (indicated by the green bar). The bar is completely grey when the memory is empty and completely green when the memory is full.
- The total memory time, in Days-Hours-Minutes-Seconds. The total memory time is displayed at the right extremity of the scale. It is calculated as a function of the instrument settings, such as log interval, statistics recorded...etc. Therefore it will change dynamically as the settings are modified, to reflect the new overall memory time.

7.3.4.1 Timer Setting

When the *Timer* button is pressed, the timer settings panel appears.

Either use the direct entry field ([Figure 6](#) (4)), or press the *Calendar View* button ([Figure 6](#) (3)) to set the date and time when the recording must start.

Press the *OK* button to exit and arm the timer.

Press the *Cancel* button, or the *Window-Close* button to exit without arming the timer.

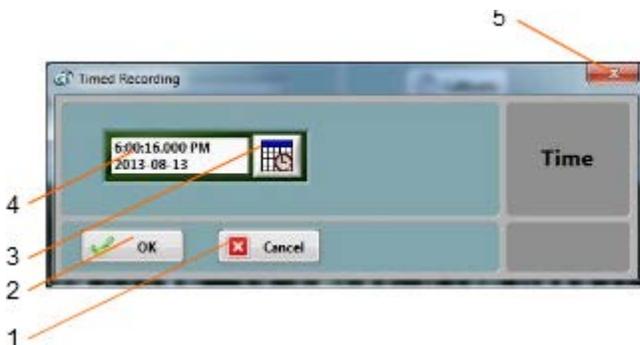


Figure 6 Timer Settings Panel

1. Cancel button – Closes the window without arming the timer
2. OK button – Closes the window and arms the timer

3. Calendar button – Brings the calendar view to enter date and time
4. Date/Time field – Can be used to enter date and time directly
5. Window close button - Closes the window without arming the timer

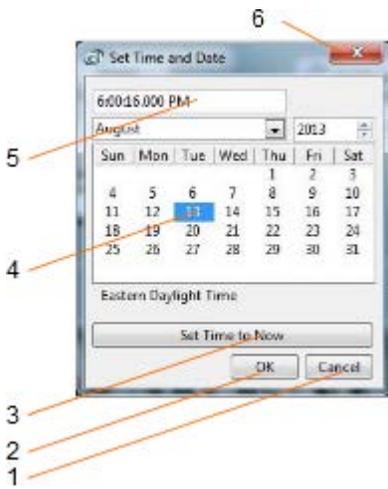


Figure 7 Calendar View

1. Cancel button – Closes the window without changing the date/time setting
2. OK button – Closes the window and accepts the newly set date/time
3. Set to Now button – Set the time and date to the present time
4. Date setting field – Click a date to set
5. Time setting field – Use the field to set a new time
6. Window close button - Closes the window without changing the date/time setting

7.3.5 Settings Field

The settings field contains the *Settings* and *Calibration* buttons.

7.3.5.1 Instrument Settings Panel

The instrument settings panel opens when the user presses the *Settings* button. Changing the settings is only allowed when the instrument is not actively recording.

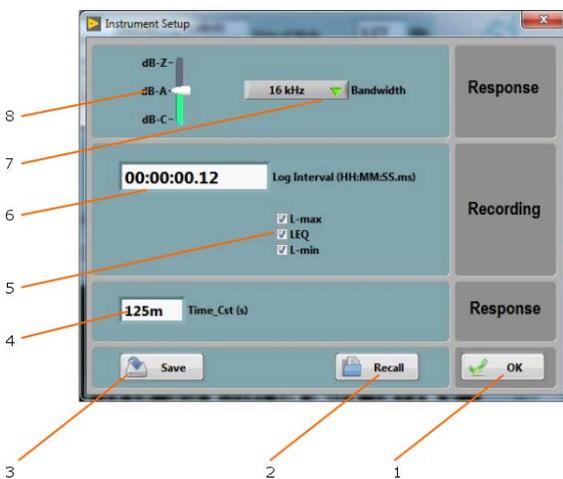


Figure 8 Instrument Settings Panel

1. OK button – Closes the window
2. Recall Button – Recalls a configuration from a configuration file
3. Save Button - Saves a configuration to a configuration file
4. Time constant for sound level measurement (only affects Lmin and Lmax)
5. Recorded Data selector
6. Log interval control
7. Bandwidth Selector
8. dB-A/dB-C/dB-Z selector

7.3.5.1.1 dB-A/dB-C/dB-Z Selector

Use this selector to choose the weighting curve. The default is dB-A, which approximates the sensitivity of human hearing.

7.3.5.1.2 Bandwidth Selector

Use this selector to choose the sampling frequency/bandwidth.

- 16 kHz bandwidth (32 kHz sampling frequency)
- 24 kHz bandwidth (48 kHz sampling frequency)

7.3.5.1.3 Log Interval

The log interval defines the time between two successive recorded points. That also defines the integration period for the LEQ, and the observation period for L-min and L-max.

The log interval can be adjusted from 125 ms ($1/8^{\text{th}}$ s) to 2 H in increments of 125 ms.

The amount of memory consumed is inversely proportional to the log interval. The *Memory-Depth* indicator in the *Setup* panel automatically calculates the overall recording time as a function of the selection.

7.3.5.1.4 Recorded Data Selectors

The recorded data selector specifies the type of statistic to record. To select a type of data, simply check the corresponding checkbox. By default, all statistics (L-min, L-max and Leq) are selected.

The amount of memory consumed while recording is proportional to the number of data types selected. The *Memory-Depth* indicator in the *Setup* panel automatically calculates the total recording time as a function of the selection.

7.3.5.1.5 Time Constant

When calculating the L-min and L-max levels, the instantaneous RMS levels are first low-pass-filtered with an adjustable time constant.

A shorter time constant should be chosen to be able to track rapid changes. Otherwise the measurements will be smoothed out. On the other hand, when the RMS levels are slowly varying, a longer time constant will provide more precise values.

Typical fast time constants are 125 ms and under. An extra fast time constant of 35 ms is sometimes used to capture L-max on very short transients.

Typical slow time constants are 1s and over.

Note: The time constant is not used for the calculation of Leq. In the case of LEQ, the sound energy is averaged linearly over the specified log interval.

7.3.5.1.6 Closing the Window

Each adjustment is implemented in the instrument when the *OK* button is pressed. If the window is closed without clicking *OK*, then the settings are not implemented.

7.3.5.1.7 Save/Recall

Once the parameters are adjusted, the whole setup can be saved to a file, to be later recalled for easier configuration.

7.3.5.2 Calibration

Note: Calibration should only be attempted if a 94dB calibrator is available. Attempting a calibration without a calibrator on the microphone will result in a complete decalibration of the instrument. When that occurs the factory must be contacted to provide the instrument's original calibration file.

The instrument can be field-calibrated using a 94 dB calibrator with a standard 1/2" opening.

Field calibration is performed by the *Instrument_Manager* application. Follow these steps:

1. Pull the wind-screen off the instrument
2. Place the instrument's microphone in the calibrator
3. Start the calibrator
4. Press the *Calibrate* button on the application window and follow the on-screen instructions.

The calibration button can also be used to recall the factory calibration in case it is lost, or the instrument is decalibrated by mistake.

7.3.6 Battery Field

This battery condition field indicates the remaining battery capacity. The indicator is surrounded by a yellow indicator that lights-up when the battery is charging.

The battery condition indicator is scaled to indicate the approximate number of days of recording time remaining in the battery.

7.3.7 Signals Field

The signals field provides information about the acoustic signal and sound level.

- The graph presents the acoustic signal as it is measured in real-time. When selected, the auto-scale button allows the scale to be dynamically adjusted so that the signal always fits in the graph. When deselected, the scale is fixed. When using a fixed scale, the scale can be adjusted manually by double-clicking and writing new values directly in the top-most and bottom-most marker values on the vertical scale. The acoustic signal is scaled in *Pascals*.
- The vertical bar to the right of the graph show the sound level measured in real time. The sound level is scaled in dB (dB-A, dB-C or dB-Z, depending on the weighting curve).

7.4 Records Tab

The *Records* tab is seen in [Figure 3](#). It is used to retrieve the recorded information from the *NSRTW_mk2* or from a saved file, and to display and optionally export the recorded logs.

7.4.1 Instrument Download

To download data from the instrument press the *Instrument Download* button. The whole contents of the instrument's memory are downloaded, and the newest record is displayed in the graph.

The *Record Selector* at the top-left of the page ([Figure 3](#) (5)) indicates how many records have been downloaded. It shows one separate tick per record downloaded. Use the white slider to select the desired record. When selecting a record the indication *No-Data* is displayed on top of any empty graph.

Note: It is legal for a record to contain no data at all. This may mean that the recording was started and stopped before any data had time to be recorded. It can also be the case if no data type (Lmin, Lmax, LEQ) was selected to be recorded. In such a case the time-stamp is still valid and can be used to determine when that recording occurred.

The *Source* indicator shows the *User-ID* of the instrument, if any has been set.

The Y-scale can be displayed in dB or linear (Pa) scale.

The graph shows up to three curves:

- L-max in red
- LEQ in white
- L-min in green

7.4.2 File Save

Pressing the *Save File* button saves all the records downloaded from the instrument to a file on the PC. In addition to the whole contents of the recording memory the file also contains ancillary information, such as calibration, instrument information...etc.

The file is saved in a proprietary format with the extension *.cil*.

By default the file is saved with a name that contains the *User-ID* of the instrument, if any has been set, as well as the present date and time.

7.4.3 File Open

Pressing the *Open File* button recalls all the records previously saved to a *.cil* or *.wlg* file. The function works very much like the *Instrument Download* function, except that the data comes from a previously saved file.

Two types of files can be opened and displayed:

- **.cil** This type of file is created by the *Instrument_Manager* application. It contains all the data that has been downloaded from the instrument.

- **.wlg** This type of file is created by the *Instrument_Listener* application. It contains data that is sent by an instrument over the network. When a *.wlg* file is opened the *Instrument_Manager* application asks to convert it to a *.cil* file.

The *Source* field shows the *User-ID* of the instrument the data comes from.

That function works even when no instrument is connected to the PC, so it can be used to examine data that was recorded elsewhere and sent to the user as a file.

7.4.4 Exporting Data

The data of the record being presently viewed can be exported for further display or processing. The data is exported to a tab-delimited text format that can be imported in *Excel* and other spreadsheet applications.

7.4.5 Global Level Calculations

The application automatically calculates the global levels or equivalent dose corresponding to the displayed data.

The global values can be calculated according to several methods. At the time of this writing we offer the linear ISO (Q=3) method, as well as the OSHA (Q=5) method. Other methods may follow.

These global values are calculated from the LEQ curve (white curve). In order to obtain the global values, the LEQ MUST BE among the recorded statistics.

The global values are calculated from the visible part of the graph only. Play with the zoom and pan functions to eliminate portions at the beginning and end of the recording from the calculation.

7.4.6 Graph Controls

The graph can be adjusted and analyzed using the following techniques:

7.4.7 Cursor Control

A cursor can be used to precisely measure the level at a particular point in time.

To the bottom-left of the graph is a three-button control. The left-most looks like a cross. In order to use the cursor proceed as follows:

- Press on the button that looks like a cross (see [Figure 3](#) (3))
- Place the mouse over the point where the X and Y cursor lines meet and left-click. This grabs the cursor.
- Drag the cursor to the specific curve and time of interest. The cursor can jump from one curve to the other.
- Read the X and Y values in the cursor field underneath the graph.

7.4.7.1 Zoom Control

To use the zoom control, simply press the button that looks like a magnifying glass and choose one of the following zoom functions:

- Zoom X-Y
- Zoom X
- Zoom Y
- Zoom-Extents

After choosing the function, the cursor changes to a magnifying glass. Click and drag on the graph to apply the required zoom.

7.4.7.2 Pan Control

To pan a graph left, right up or down, first press on the *Hand* button to the left of the graph. Then position the mouse over the graph. Left-click to “grab” the graph, and move the mouse to pan the graph as desired.

7.4.7.3 X-Y-Scale Direct Modification

Another way to zoom a graph is to directly change its scale. To do that, simply click on the value for left-most or right-most marker of the X-scale, and select its value. Type a new value to replace the old one. The scale is adjusted so that that new value is used at the beginning or end of the scale.

The same technique can be applied to the bottom-most or top-most values of the Y-scale of the graph.

7.5 Spectrum Tab

The *Spectrum* tab is shown on [Figure 4](#). When that tab is selected the time-domain signals captured by the instrument are presented in the form of averaged power spectra. The processing is as follows:

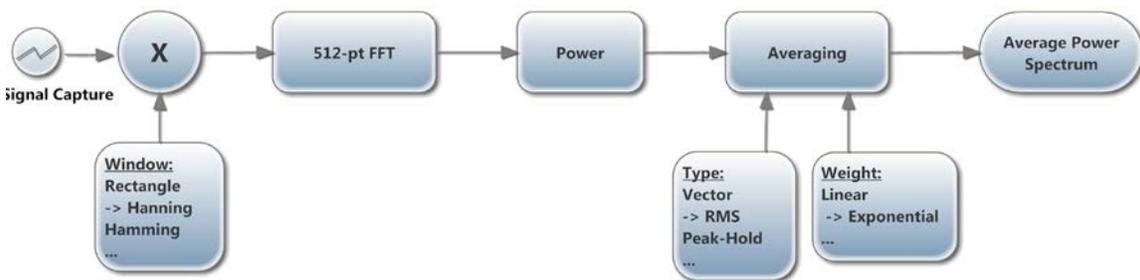


Figure 9 (-> shows the defaults)

7.5.1 Window

The type of window chosen has an impact on the spectral resolution. The *Hanning* window is generally a good choice that provides good spectral selectivity.

7.5.2 Weighting

The averaging can be exponential or linear.

- **Exponential Averaging** is comparable to a low-pass time filtering of the spectrum. In other words each spectral line is low-pass filtered so that the resulting spectrum is smoothed out over time. In that case the *Nb_Avg* represents an equivalent averaging time constant, expressed in number of successive spectra. The averaging is continuous and does not stop. Each successive spectrum is taken into account in the calculation. A larger value of *Nb_Avg* produces a spectrum that is more stable, but also averages-out short-lived transients.
- **Linear Averaging** takes an equal-weight average of *Nb_Avg* successive spectra. After the *Nb_Avg* spectra have been observed the result is frozen.

In both cases the *Reset* button discards the present display and restarts the averaging from zero.

The *Averaging Mode* can be chosen from several choices:

- **RMS Averaging** RMS averaging reduces signal fluctuations but not the noise floor. The noise floor is not reduced because RMS averaging averages the power of the signal. *RMS Averaging* is the most common type.
- **Peak-Hold** Peak hold averaging retains the peak levels of the measured spectra. Peak hold averaging is performed at each frequency line separately, retaining peak levels from one FFT record to the next.

Note: All the FFT calculations are performed on the PC. The raw time-signals are transferred from the instrument to the PC, where the FFT and averaging calculations are performed.

7.5.3 Scale

The power spectra can be displayed in dB or linear (Pa) scale. Changing the scale does not restart the averaging.

7.5.4 Cursor, Zoom and Pan

Cursor, Zooming and Panning is done the same way as in the *Records* graphs. See section [Graph Controls](#)

The auto-scale button can be pressed or released to obtain an automatic or fixed vertical scale. When the graph is in fixed scale, writing directly in the values of the end-scale markers sets the scale to fit those values.

7.6 WiFi Tab

The *WiFi* tab has all the indicators showing the instrument's present state of connection, as well as controls to configure *WiFi™* and email settings.

7.6.1 Connection Status

7.6.1.1 Levels of Connection

When trying to connect, either at the preset interval, or for an email alarm, the instrument will do it in two stages:

- The instrument first tries to connect to a *WiFi™* router or access-point in its vicinity.
- Once connected to the network through the router or access-point, the instrument will then try to connect to a server (either the specified email server, or the server running the *Instrument_Listener* application, depending if that is an alarm or part of the regular reporting of

recorded levels. The server connection can be done to a specified IP address, or to a domain name. Connecting using a domain name is preferable because IP addresses are often subject to change.

The instrument has a total time of 1 minute to go through the two stages. If the final stage is not established by the end of that minute, the instrument stops trying in order to preserve battery. It will then retry at the next preset interval, or if a new email alarm is triggered.

Note: In order to maximize data throughput and minimize power consumption, it is best to locate the router or access point close to the instrument so WiFi™ communications are reliable.

Note: If the Instrument_Listener application is not running on the server, the instrument will not be able to download any data.

Note: The panel shown in [Figure 5](#) will display the progression of the connection when the instrument is connected through USB. It is designed to help debugging connection problems

The *Connection Status* field indicates graphically the different stages of connection. Each icon (7, 8, 9 and 10 in [Figure 5](#)) indicates a different connection stage:

- Indicator 7 Active: The instrument is actively trying to connect to a Router or Access-Point
- Indicators 7 and 8 Active: The instrument is connected to a Router or Access Point. In this case the SSID of the Router or Access Point is written in indicator 5.
- Indicators 7, 8 and 9 Active: The instrument is on the network.
- Indicators 7, 8, 9 and 10 Active: The instrument has connected to the server and is talking to the *Instrument_Listener* application. In that case the server's IP address is written in indicator 11.

7.6.2 WiFi Settings

The *WiFi* settings panel appears when the *Set WiFi* button is pressed. The *WiFi* settings are used to configure the Router(s) or Access Point(s) to connect to, the Server's IP address or domain name, and the periodic connection schedule.

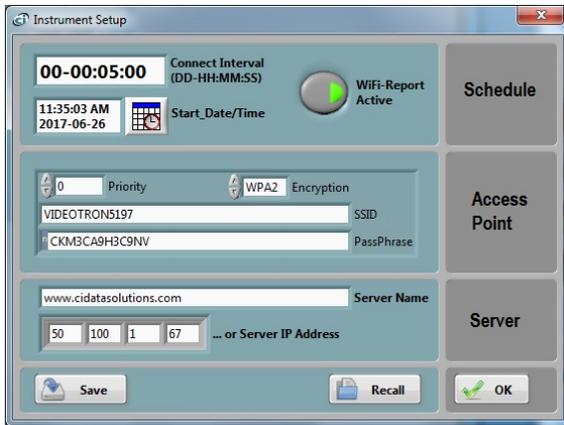


Figure 10 WiFi Settings

7.6.2.1 Schedule

Whether it is recording or idle, the instrument can activate its *WiFi™* interface and try to connect to a server at regular intervals. The connection schedule is defined in that field. In order to enable that behavior, the following must be setup:

- The Connect Interval must be set:** The interval is often chosen as once per hour, or once per 10 min. Setting a very small interval will let the instrument report much more often, but that will drain the battery faster. Setting a much longer interval (several days, a week or more) will risk losing data if the connection cannot be established at its scheduled time. The interval must not be set as 0. We do not advise setting a schedule interval lower than 2 min.
- The *WiFi-Report-Active* button must be pressed:** When the button is released the instrument will not try to connect at the set interval.
- A start date and time must be set sometime in the future:** The periodic connection attempts will only begin at the set date and time.

7.6.2.2 Access Point

The coordinates the access point or *WiFi™* router can be set, with its security method, password, and priority. Each router or access point is defined by its *SSID*.

When security is used, a password must be entered.

Note: By clicking on the little grey block at the left of the pass-phrase field, several input methods can be selected:

- Password (P)* is used to conceal the password being entered
- Hex (H)* is normally used in conjunction with WEP security
- Normal (N)* is normally used in conjunction with WPA and WPA2 security

7.6.2.3 Server

The server can be defined by its IP address, or its domain name. This server can reside on the local network, or on the internet. Once the instrument is connected to the access point, it will attempt to contact the IP address of the server.

Note: When the server is not on the local network, the configuration of the router it is connected to is more complicated. See section [7.6.4](#).

7.6.3 Manual Connection

In order to test the *WiFi™* connection, after setting up the Router or Access-Point and/or the server's IP address or domain name, but prior to setting a connection schedule, press the *Connect-Now* button. The connection status will show that the instrument is immediately trying to connect, and will show all the connection stages in sequence.

In order for the last stage (Server Connected) to be reached the server must be working, must be reachable, and must be running the *Instrument_Listener* application.

7.6.4 Setting Up the Server to Work in a Local or Wide Area Network.

Setting up a server to run on the same local network the instrument is in is relatively easy. In addition to the steps above, one should make sure of the following:

- The IP address of the PC working as a server must be fixed. To that end, the router that the PC is connected to must be set to use "Static DHCP" for that PC. This way the IP address cannot change.
- The PC working as a server must be always on, and must be running the *Instrument_Listener*. Otherwise the connection can't be established when the instrument tries to connect.

Setting up a server to work in a Wide Area Network (in a different city for instance) is a little more complicated. One option is to use a corporate server running the *Instrument_Listener*. In that case it usually makes sense to use a domain name to represent the server's address.

When the server is a simple PC in an office, the following configuration may be used:

- The router that the PC is connected to is configured for "Port Forwarding". Port Forwarding must be enabled on port 50 000, for TCP/IP, to the local IP address of the PC.
- Static DHCP must be configured on that PC, so its local IP address will not change.
- Ideally the router must be setup to use a DDNS service, such as *noip.com*. This way the instrument can use a domain name registered through the DDNS service in order to contact the server. Alternately the instrument's server setup can use the WAN IP address of the router that the server is connected to. That is a less optimal solution because that WAN IP address is often subject to change by the internet provider, and when it changes the instrument won't be able to connect to the server anymore.

7.6.5 Email Setup

Email alarms can be setup by pressing the *Set* email button.

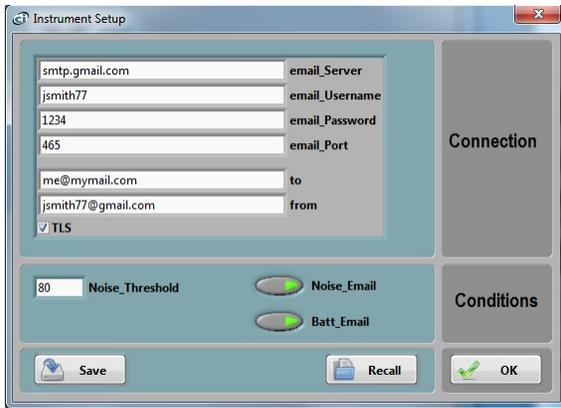


Figure 11 Email Setup

Email alarms require the following conditions:

- The *WiFi* setup must have already been done so the instrument can connect to a router or access point.
- That router or access point must be connected to the internet.
- The user must have an email account to use for outgoing email. A good solution is to use a *gmail* account.

The email setup is not always easy. See https://convergenceinstruments.com/pdf/Gmail_Setup.pdf for details.

The complete email setup is similar to the configuration of any email application. It includes the following:

- **Email server** The internet name of the outgoing email server. For gmail this is *smtp.gmail.com*
- **Port number** The TCP port number of the email service. This is usually:
 - **25** for an “open” (no security) account.
 - **465** for SSL security
 - **587** for TLS security
 For gmail this is port 587 or 465.
- **User-name** The account name. For gmail it is the user’s account name (to the right of the @ sign).
- **Password** The account password (leave blank for an “open” (no security) account). For gmail this is the password.
- **TLS** The encryption setting. This is the only secure mode supported. Uncheck for an “open” (no encryption) account. For gmail this should be set.

In addition to these settings, the email alarms settings let you set:

- **One Recipient** The recipient line (*to* line in [Figure 11](#)).
- **The sender’s address**

The application by default shows the settings for a fictitious secure *gmail* account (see [Figure 11](#)). These settings of course need to be changed to reflect the user's own email account settings.

In addition see https://convergenceinstruments.com/pdf/Gmail_Setup.pdf for additional settings of the *gmail* account itself.

Two types of alarms can be sent:

- An alarm when a set noise threshold is exceeded
- An alarm when the battery level is too low. The level cannot be adjusted. It is set so the instrument has enough reserves to send the alarm.

7.6.6 *WiFi*TM Battery Drain

Connecting to a network drains the battery. Even if the instrument is idle, if the periodic connection is enabled, the instrument will regularly wake up and attempt to connect to the server. Trying to connect at regular intervals will drain the battery in a short amount of time.

When that behavior is unwanted (for instance when the instrument is unused and in storage) pressing the *Disable All* button (see [4 Figure 5](#)) will completely disable *WiFi*TM and email connectivity. If the instrument is idle with all its *WiFi*TM connectivity disabled, it can keep its battery for at least 6 months.

8 Instrument_Listener Application

In order to report recorded data, and send alarm emails, the instrument must connect to a remote PC (a server) that is running the *Instrument_Listener* application. The *Instrument_Listener_Installer_Vxxx* must be installed on the PC (*Vxxx* represents the version number of that application).

The remote PC (the server) must:

- Be on
- Be reachable over the network, either by an instrument on the local network, or on a global network. In the case of a global network, all firewalls must allow the server to receive incoming connections.
- Be running the *Instrument_Listener* application. It may be useful to setup that application so that it runs automatically when the PC boots.

The *Instrument_Listener* application (see [Figure 12](#)) always listens to incoming connection attempts from instruments in the field. Whenever an instrument tries to connect, it opens an *NSRTW_Server* window (see [Figure 13](#)). That window briefly opens to show the communications with the instrument, battery level and temperature. It manages all operations that the instrument needs to perform and then closes back down.

Note: When several instruments try to connect at the same time, the Instrument_Listener application will open multiple NSRTW_Server windows.



Figure 12 Instrument_Listener Application

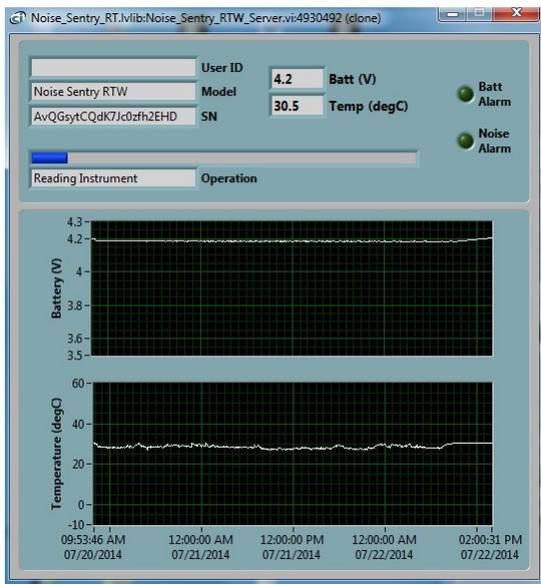


Figure 13 NSRTW_Server Window

The *NSRTW_Server* window performs the following operations:

- If data is in the instrument, it creates a *.wlg* file to hold that data, or appends the data to the file if one has already been created.
- If the instrument is not currently recording, it then erases the instrument's memory, adjusts the time, and starts recording. If the instrument is recording it closes as is and lets the recording continue.

8.1 File Storage

The *.wlg* files that are created by the *NSRTW_Server* are stored in *C:\Users\username\Documents\Convergence_Instruments\All_Instruments\Records\NSRTW_mk2*, where *username* is the name of the user currently logged. In the context of a particular user's account, this folder is normally designated:

Libraries\Documents\My Documents\Convergence_Instruments\All_Instruments\Records\NSRTW_mk2

These *.wlg* files can be opened for viewing by the *Instrument_Manager* application. When they are opened the application will ask to convert them to a *.cil* file. The *.cil* format is easier to open, and can be opened by other applications in the suite.

9 Maintenance

9.1 Battery Care

The following factors affect battery life:

- Prolonged use at extreme temperatures (close to the limits of $-20\text{ }^{\circ}\text{C}$ and $+60\text{ }^{\circ}\text{C}$ ($-4\text{ }^{\circ}\text{F}$ to $140\text{ }^{\circ}\text{F}$) will shorten the life of the battery.
- Over-discharge of the battery will shorten the life of the battery. Always fully recharge the battery when it is low or at least every 6 months, whichever comes first.
- Never leave the instrument in storage with the *WiFi™* set to periodically connect.

9.2 Reset Procedure

In the unlikely case where the instrument's firmware crashes a hardware reset can be performed by inserting a small rod into the reset hole and pushing until a slight click is felt. There is no risk of losing any recorded data or settings by resetting the instrument. However a hardware reset will reset the instrument's time and date to a value in year 1903.

9.3 Operation Outdoors

Thanks to its potted construction, the *NSRTW_mk2* is weather-proof. It can safely be used outdoors provided that the temperature is always within the safe limits. However when using it outdoors with a risk of rain or snow, make sure its USB connector is facing down, so water will not accumulate in the connector and microphone port.

9.4 Dust

The instrument is designed to work outdoors, under the rain, snow...etc. But its microphone is sensitive to dust. When working in dusty environments, please see the white paper: https://convergenceinstruments.com/pdf/Dust_Issues.pdf

9.5 Cleaning

Use a damp sponge or soft cloth.

Note: Do not use solvents.

Do not submerge in water.

Do not blow onto or near the microphone

9.6 Software and Firmware Upgrades

Software upgrades are found on our web site: www.convergenceinstruments.com.

After upgrading the software, if a firmware upgrade is required it will be applied automatically when the upgraded *Instrument_Manager* application is started. In that case do not disconnect the instrument until the upgrade is completely over. Failure to do that will place the instrument in a state where it no longer works.

Note: A firmware upgrade will not lose any recorded data, but will reset the instrument's settings.

Note: When upgrading the instrument's firmware always make sure that only one instrument is connected to the PC at a time.

10 Troubleshooting

10.1 USB Power Limitation

In some instances a PC will not allow the instrument to connect to one of its USB ports because it cannot provide the battery charge current requested by the instrument. If you suspect that this may be a factor, try connecting the instrument to the output of an externally-powered USB hub that is capable of providing a full USB load (500 mA).

10.2 USB Driver Installation

If the *Instrument_Manager* application is unable to communicate with the *NSRTW_mk2* it may be because the USB driver failed to install properly. To check the USB driver installation follow the procedure below:

1. Disconnect the USB cable.
2. If necessary take the PC out of stand-by.
3. Reconnect the instrument to an available USB port on the PC.
4. Make sure the charge LED lights-up green (charged) or yellow (charging). If not, make sure that the PC's USB port is functional and that the USB cable is not damaged. If necessary try on a different PC, and/or with a different USB cable. The charge LED is just an indication that the port is powered. It should light-up, even if the USB driver is not installed properly.
5. Make sure that the operation LED starts blinking. If not go to step 6.
6. Open the *Device Manager* on the PC. This is usually found in *Control Panel – System and Maintenance*.
7. Just after connecting the instrument to the PC, observe that the *Device Manager* window refreshes.
8. Verify that an item named *DDCI Platform* or *NSRTW_mk2* has been created in the list of devices.
9. If an unknown item appears, or an item named *DDCI Platform* or *NSRTW_mk2* is found but has an exclamation mark (indicating a problem) beside it, disconnect the device and try re-installing the driver (see step 10).
10. To re-install the driver disconnect the *instrument from the PC*. Then Go into *Start\All Programs\Noise_Sentry_RT_Management\Driver*, and run *DDCI_Driver_Install.exe*. This re-installs the USB driver.

10.3 Connection Problems

Failure to communicate with the PC can also be caused by poor USB cable contacts. Make sure the USB connector is fully inserted into the socket of the *NSRTW_mk2*. Inspect the inside of the socket in the instrument. If dirt is lodged in the socket, use dry compressed air to expel it.

Make sure not to blow air at or near the microphone!